

Scrambler therapy

A. F. SABATO ¹, G. MARINO ², A. CATU ¹

*Anesthesiology and Resuscitation Unit
Service of Physiopathology and Therapy of Pain
Department of Anaesthesia
Tor Vergata University, Rome, Italy
*Data Research and Development
Medical Engineering Research Centre
Rome, Italy*

In neuropathies there are complex reactions that modify the homeostatic equilibrium of pain system. In such a context the Scrambler Therapy (ST5) interferes with pain signal transmission, by "mixing" a "non-pain" information into the nerve fibres. The aim of this study is to evaluate the effectiveness of ST5 in the treatment of neuropathic pain. The ST5 consists of a multiprocessor apparatus able to stimulate 5 artificial neurons by the application of surface electrodes on skin pain areas. A total of 226 patients, all suffering from intense drug resistant neuropathic pain, were recruited for this trial in 2004. Inclusion criteria: neuropathic pain, very high baseline visual analogue scale (VAS). Exclusion criteria: pacemaker users, neuroleptic blocks or neuroleptic pain control treatment. The treated neuropathic pain syndromes were: failed back surgery syndrome (FBSS), sciatic and lumbar pain post herpetic (PHN), trigeminal neuralgia, post-surgery nerve lesion neuropathy, podotal neuropathy, brachial plexus neuropathy, low back pain (LBP), others. The trial programme: 1 to 6 therapy sessions of 5 treatments, each one lasting 30 min. Pain intensity was evaluated using VAS before and after each treatment. The statistical significance of VAS was measured using the paired *t* test. The total results show 80.09% of responders (pain relief >50%), 10.18% of par-

tially responders (pain relief from 25% to 49%) and 9.73% of no responders (patients with pain relief <24% or VAS >3). The conclusion is drawn that ST5 produced a statistically significant ($P < 0.0001$) pain relief in all treated neuropathies.

Key words: Scrambler therapy - Pain - Neuropathies.

The pain system is characterized by a high level of information content. Specific receptors, mechanoreceptors and multimodal receptors, respond indifferently to all painful stimuli; they are biological elements that are able to transduce a chemical, physical or mechanical event into specific pain information. The complex modifications activated by the nervous system in response to a painful stimulus are the focus of a wide variety of reactions designed also to reestablish conditions of homeostatic equilibrium that the pain information signals have provoked. In most cases, this equilibrium can be rapidly restored thanks to a series of reactions involving much of the biological sys-

¹ Research supported by the Unit of Anesthesia, Analgesia and Resuscitation, Tor Vergata University of Rome and the Data Research & Development, Medical Engineering Research Centre, Rome, Italy

Address reprint requests to Prof. A. F. Sabato, Via Mazzini 153, 00144 Roma, Italy
E-mail: sabato@med.uniroma2.it




Figure 1. Causes/pathology (total 225).

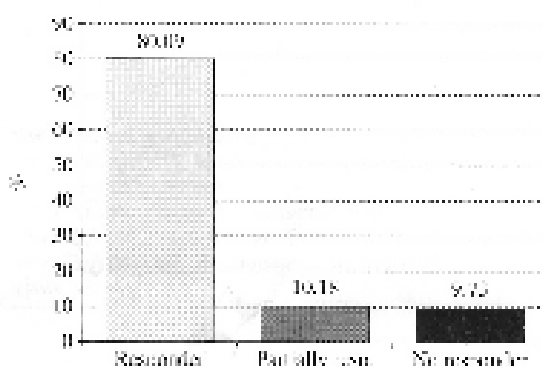


Figure 2. Post-operative responses.

tem as a whole. However, there are situations in which this has not happened, either due to the impossibility of removing the cause, or due to intrinsic damage to the pain system itself (neuropathies). In such a context, complex reactions may modify the original information triggering the pain phenomenon (sensitization), thus setting up an iterative process that, in the case of chronic pain, and of neuropathic and visceral pain in particular, tends to render all known therapeutic strategies gradually (or completely) ineffective. The useful fact that emerges from all these scenarios is the central role of control exercised by information over the chemical-structural variations of the system. In this case, information is represented by the sequence of pulses generated by the activated nociceptor, pulses that "describe" the type of pain. Overall, this represents a good description of a cybernetic process: communication (pain information) and regulation (chemical feedback to modify percep-

tion and adaptive reactions). It may thus be reasonably assumed the possibility to control the lower levels of complexity of the pain system (the chemical reactions) by manipulating the "information" at higher levels. The incomplete knowledge characterizing the role of the chemical molecules involved in the pain phenomenon may conveniently be represented by the black box technique. This involves a model in which the input and output are known, but not the internal translation process that takes place inside the "box".

The research procedure adopted, therefore, allowed a comparatively complex system model, in which the biological variables were translated into cybernetic variables, extrapolating the role and the modality of the pain information, regardless of the biochemical aspects and its etiopathogenesis.

The approach actually adopted to respect the initial theoretical criteria (use of information as the active principle) was to replace the "pain" information with artificial "no-pain" information, in full respect of the information theory. Essentially, an artificial neuron was developed that behaves as a "Pain Scrambler". This system is able to interfere with pain signal transmission, by "mixing" a "no-pain" signal, into the transmission channel (the nerve fibres), for the purpose of masking the original pain information. The "no-pain" signal is still recognized as "self" by the nervous system.¹⁻⁴

The aim of this study was to evaluate the effectiveness of Scrambler Therapy (ST) in the treatment of neuropathic pain.




Figure 3. —VAS pre- and post-session.

Materials and methods

The STS consists of a multi-processor apparatus able to simulate 5 artificial neurons that allow 5 pain areas in the same person to be treated simultaneously. The treatment is fully automated, including the dynamic parametrization required for the correct functioning of the method. This criterion ensures a very high degree of repeatability of the experimental data, as it is not necessary to select the operating parameter manually except for the simple regulation of stimulus intensity, which is manually set at the perception threshold. Each treatment session lasts 30 min on average. Application is by means of disposable surface electrodes applied in the skin areas corresponding to the pain areas.

A total of 226 patients, all suffering from intense drug-resistant neuropathic pain, were recruited for the trial in 2004.

Inclusion criteria:

- neuropathic pain;
- very high baseline visual analogue scale (VAS) in drug treatment.

Exclusion criteria:

- pacemaker user;
- neuroleptic blocks or neurolesive pain control treatment.

The trial programme was based on a series of therapy sessions: from 1 to 5 cycles of 5 treatments every 24 h.

Figure 1 shows the number of treated patients suffering from neuropathic pain syndromes: failed back surgery syndrome (FBSS) (45 patients), sciatic and lumbar pain (33 patients), post-herpetic neuralgia (PHN) (21 patients), trigeminal neuralgia (20 patients), post-surgery

nerve lesion, trigeminy (21 patients), podiatric neuropathy (11 patients), brachial plexus neuropathy (12 patients), low back pain (LBP) (14 patients), others neuropathies (46).

The patients were stratified in 3 groups: responders patients - pain relief >50%, partially responders: pain relief from 25% to 49% and no responders patients - pain relief <24% or VAS >5.

Pain intensity was evaluated using VAS before and after each treatment. The statistical significance of VAS was measured using the paired *t*-test.

Results

Figure 2 shows total percentage responses: 80.09% of patients was responder, 10.18% was partially responder and 9.73% was no responder.

The VAS trends before and after the treatment sessions are shown in Figure 3: in FBSS the VAS decreases from 7.01 to 2.79; in lumbar and sciatic pain from 5.61 to 1.82; in PHN from 6.45 to 2.73; in trigeminal neuralgia from 6.41 to 1.89; in post-surgical pain syndrome from 7.07 to 2.33; in the damage of brachial plexus from 7.23 to 2.42; in the damage of podiatric nerve from 6.82 to 3; in LBP from 6.53 to 2.55.

All VAS values are statistically significant ($P < 0.001$).

Conclusions

The following conclusions may be drawn from these results:

— ST5 produced a surprising statistically significant ($P < 0.001$) pain relief.

— No undesirable side effects were reported.

All the patients displayed excellent compliance with the treatment.

This extremely positive outcome is an encouragement to perform more extensive trials of Scrambler Therapy to obtain further knowledge.

Riassunto

Scrambler therapy

Nelle neuropatie ci sono complesse reazioni che modificano l'equilibrio eccitatorio del sistema del dolore. In questo contesto la Scrambler Therapy (ST5) interviene con la trasmissione del segnale del nocice, inserendo un'informazione di "non dolore" nelle fibre nocice.

Lo scopo di questa studio è stato valutare l'efficacia della ST5 nel trattamento del dolore neuropatico.

La ST5 è un dispositivo multiprocesso, capace di simulare 5 canali artificiali attraverso l'applicazione di elettrodi superficiali su aree cutanee dolenti.

Nel 2009 sono stati reclutati per lo studio 226 pazienti, u.t. affetti da dolore neuropatico farmaco-resistente. Criteri di inclusione: dolore neuropatico, scala visiva analogica (VAS) con valore iniziale molto alto. Criteri di esclusione: portatori di pacemaker,

blochi nervosi o trattamenti neurolesivi per il controllo del dolore.

Le neuropatie trattate sono state: failed back surgery syndrome (FBSS), mioposciatalgia, neuralgia post-erpetica (post-herpetic neuralgia, PHEN), neuralgia del trigemino, neuropatia post-ictologica, neuropatia del polsone, neuropatia del plesso brachiale, low back pain (LBP) e altre.

Il protocollo da 1 a 6 cicli terapeutici di 5 minuti, ciascuno della durata di 30 minuti.

L'intensità del dolore è stata valutata mediante VAS prima e dopo ciascun trattamento. La significanza statistica della VAS è stata valutata usando il t-test.

Risultati finali mostrano un 80,09% di risposta (riduzione del dolore >50%), 10,18% di pazienti con le risposte (riduzione del dolore compresa tra 25% e 45%) e 9,73% di non risposta (riduzione del dolore <25% o VAS >5).

Sulla base dei risultati gli Autori raccomandano che la ST5 produce una riduzione del dolore statisticamente significativa ($P < 0,001$).

Parole chiave: Scrambler Therapy - Dolore - Neuropatie.

References

1. Sensiini T, Van Kooij Salas AE. Scrambler Therapy: a new option in neuropathic pain treatment. *Pain Clin* 2009;12:2-1-3-9.
2. Giamberini G, Spazzoni A, Galati A, Minicini F. A new method for chronic neurological pain: the potential of Scrambler Therapy to modify a biological information. *Int Congr Ser* 2003;1477:261-6.